


STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENTATION SERVICE REPORT

1. Department: Wall Township Police Department 2700 Allaire Road Wall, NJ 07719		2. Contact: Ptlm. Adam Cox	4. Date: 01/23/2023
		3. Phone Number: (732) 449-4500	5. County: Monmouth
6. Alcotest Instrument Serial Number: ARMH-0017	7. Simulator Component Serial Number: N/A	8. Temperature Probe Component Serial Number: N/A	

9. Reason for Service:
Complaint received of the instrument displaying the message ERROR 109 EC SYSTEM, HARDWARE ERROR CALL 201.

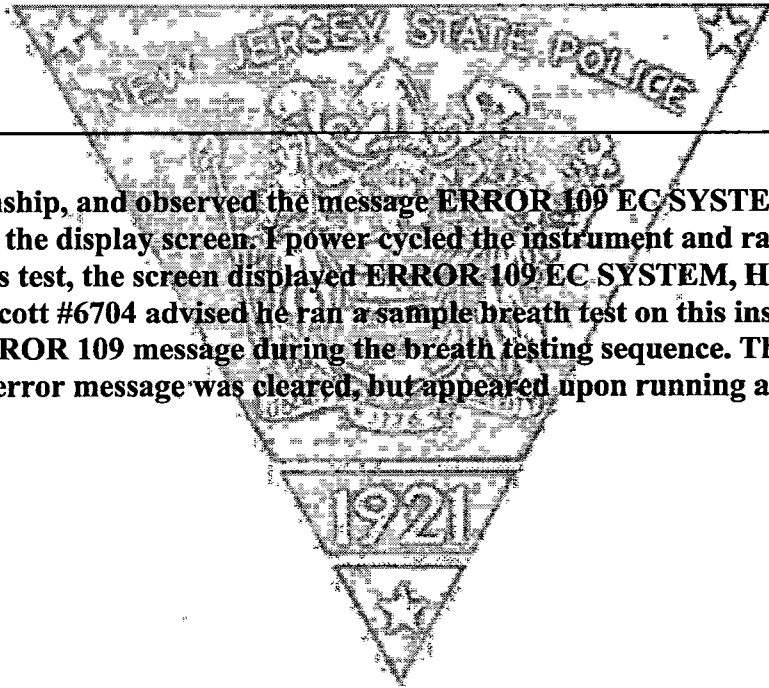

10. Comments:
I arrived at Wall Township, and observed the message ERROR 109 EC SYSTEM, HARDWARE ERROR CALL 201 on the display screen. I power-cycled the instrument and ran a cal check of the instrument. During this test, the screen displayed ERROR 109 EC SYSTEM, HARDWARE ERROR CALL 201. SFC. K. Alcott #6704 advised he ran a sample breath test on this instrument, and it displayed the same ERROR 109 message during the breath testing sequence. The instrument was power cycled, and the error message was cleared, but appeared upon running a test.

Last Known Sequential File #: 00137

- 11. The above Instrument/Component has been found to be in satisfactory working condition; no further action required.
- 12. The above Instrument/Component is placed out of service pending further evaluation.
- 13. The above Instrument/Component is placed back in service.

"I have been certified by the Attorney General as a Breath Test Coordinator/Instructor pursuant to N.J.A.C. 13:51, et. seq. In my official capacity as a Breath Test Coordinator/Instructor I perform inspections of evidential breath test devices and related components of evidential breath test systems. I have inspected the evidential breath test device listed on this report in my official capacity. The results of my inspection are recorded on this form. I certify that the forgoing statements made by me are true and accurate to the best of my knowledge. I am aware that if any of the forgoing statements made by me are willingly false, I am subject to punishment."


Tpr II. Nicholas E. Mimikos #7413	TPR II. <i>A. Mimikos</i> #7413	1/23/2023
Name & Badge Number (Print)	Signature	Date

STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENTATION SERVICE REPORT

1. Department: Wall Township Police Department 2700 Allaire Road Wall, NJ 07719		2. Contact: Ptlm. Adam Cox	4. Date: 05/18/2023
		3. Phone Number: (732) 449-4500	5. County: Monmouth
6. Alcotest Instrument Serial Number: ARMH-0017	7. Simulator Component Serial Number: N/A	8. Temperature Probe Component Serial Number: N/A	

9. Reason for Service:
The alcotest instrument was returned from outside evaluation and placed back in service.

10. Comments:
See Draeger Return and Repair Form

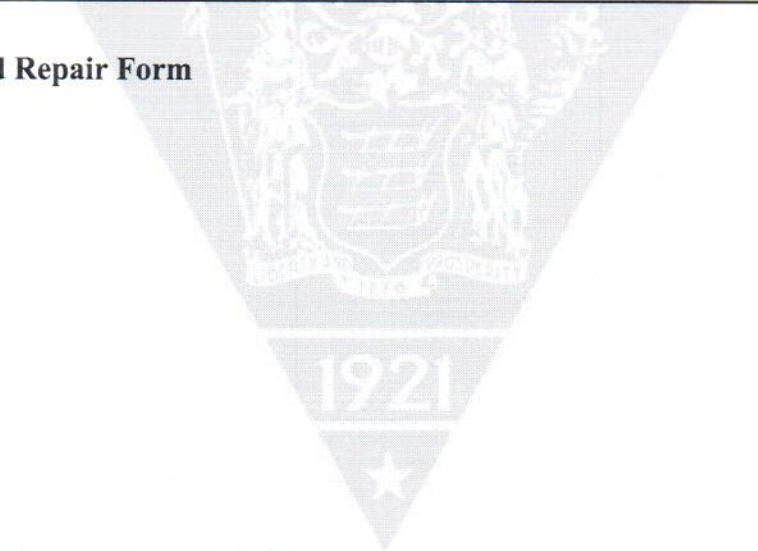

Last Known Sequential File #: N/A

- 11. The above Instrument/Component has been found to be in satisfactory working condition; no further action required.
- 12. The above Instrument/Component is placed out of service pending further evaluation.
- 13. The above Instrument/Component is placed back in service.

"I have been certified by the Attorney General as a Breath Test Coordinator/Instructor pursuant to N.J.A.C. 13:51, et. seq. In my official capacity as a Breath Test Coordinator/Instructor I perform inspections of evidential breath test devices and related components of evidential breath test systems. I have inspected the evidential breath test device listed on this report in my official capacity. The results of my inspection are recorded on this form. I certify that the forgoing statements made by me are true and accurate to the best of my knowledge. I am aware that if any of the forgoing statements made by me are willingly false, I am subject to punishment."

<p><u>Tpr I. Nicholas E. Mimikos #7413</u> Name & Badge Number (Print)</p>	<p><u>TPRI.  #7413 5/18/2023</u> Signature Date</p>
--	---

RETURN AND REPAIR FORM



Customer Information

B:

S:

Company Name: Township of Wall, Wall Township, NJ

Date Received: 01/30/2023

Date given to service: 01/30/2023

Carrier: FedEx UPS USPS Shipping Method: GRD 3DAY 2DAY
 NDA-PRI NDA-STD

Product: 6510 6810
 7110 8610
 7510 DT5000
 7410 Upper-half 9510
 7410 Whole

Serial Number: AR MH-0017

Printer Serial#: AR

Sim Serial#: DD

Probe Serial#: DD

Warranty Expires: _____

Description: A B Plus Demo Screener Trade In

Accessories

110V A/C Adapter Regulator Printer Ribbon Printer Paper
 Mouthpieces 9510 Stylus 9510 Top Cover Carrying Case
 Dry Gas Other (please specify) _____

Repair Information

Test#: _____

Part Number	Description	Qty	Total Cost
MP Cal 71	Calibration	4.0	
MP Labor	Labor	0.5	
6808550	EC sampling system	1	

Repair Notes: EC System requires replacement. QC and testing complete. No errors after repairs.

FUEL CELL = ARMF-1910
CAL W/QC AND OPS CHECK

Service Technician MB/GR

Date: 05/05/2023

Delivery receipt



Customer no.
150062190

Number of report
307918955
Please reference on inquiries

Date of receiving Delivery receipt date
/ / 05/11/2023

Consignee, 150062190
TOWNSHIP OF WALL POLICE DEPT
PTL. ADAM COX #164
ARMH-0017
2700 ALLAIRE RD
WALL TOWNSHIP NJ 07719-9570

Customer, 150062190
TOWNSHIP OF WALL
PAM KING
ARMH-0017
2700 ALLAIRE RD
WALL TOWNSHIP NJ 07719-9570

Your order

Date of order:
02/23/2023
Purch.ord.no.:
ARMH-0017

Branch text

Draeger contact person

Service Support-IDT
800-437-2437 OPT 5
SS-IDT@draeger.com

Page 1

Quantity	Description	Part no.	Equipment - No.	Serial - No.
	Alcotest 9510 New Jersey	8327998	1027996146	ARMH-0017
	REPAIR ARMH-0017			

Draeger Inc.
Our Tax ID: 23-1699096
3135 Quarry Road, Telford, PA 18969
An Equal Opportunity Employer M / F / V / H
Telephone 800-437-2437
<http://www.draeger.com>

Remit to:
LOCKBOX (Standard USPS)
Draeger, Inc.
PO Box 13369
Newark, New Jersey
07101-3362

Remit to:
LOCKBOX (Overnight)
FIS Lockbox Processing
Lockbox #13369
100 Grove Road
Suite E
West Deptford, NJ 08066

Remit US Wire Transfers to:
Account Name: Draeger Inc.
Account Number: 00-494-936
Transit Routing: 021001033
SWIFT: BKTRUS33
Deutsche Bank Trust Company Americas
60 Wall Street 25th Fl, New York, NY 10005

Service note

Customer no. 150062190
Number of report 307918955
Date of receiving 05/01/2023
Please reference on inquiries

Customer
TOWNSHIP OF WALL
2700 ALLAIRE RD
WALL TOWNSHIP NJ 07719-9570

Consignee
TOWNSHIP OF WALL
2700 ALLAIRE RD
WALL TOWNSHIP NJ 07719-9570

Your order

Date of order:

02/23/2023

Your reference:

ARMH-0017

NL-Text

UPDATE ON REPAIR WKFLO#004196

Your contact person

Service Support-IDT

800-437-2437 OPT 5

SS-IDT@draeger.com

Page 1

Item	Quantity	Part no. Description
		Service Order: 148242358
		REPAIR ARMH-0017
		Eq.No. : 1027996146 SN: ARMH-0017
		Material: 8327998 Alcotest 9510 New Jersey
		Inv.No. :
		Location:
		REPAIR ARMH-0017
		REPAIR ARMH-0017
	0.5 H	R001 Repair time - normal hours